DL76



DATA LOGGER SYSTEM INSTRUCTIONS



GENERAL INFORMATION

The DL76 is a battery-powered data logger that can be used with any Seametrics flowmeter. It stores pulses for up to 3 years, depending on the user-selected frequency of reading. Indicator lights on the unit flash to indicate when it is functioning and when the battery is low.

The DL76 can be factory-mounted on the meter or remotely mounted. Housings are rugged cast aluminum, gasketed for environmental protection.


When a DL76 logger is placed into operation, it is easily set up using a laptop computer. Data is also retrieved from the

FEATURES

DL76 by means of a laptop and can be analyzed on the laptop or easily loaded on a desktop computer for analysis.

FlowInspector software (ordered separately) is required for the downloading, storing, viewing, graphing, charting and printing of data in several formats.

FlowInspector requires a PC with Windows 98, NT, 2000, XP, Vista, or Windows 7; CD-Rom drive; 800 x 600 screen resolution; serial port or USB/serial adapter; and a Seametrics DC3 data cable. FlowInspector comes in versions compatible with up to 4, up to 16, or 17+ dataloggers.

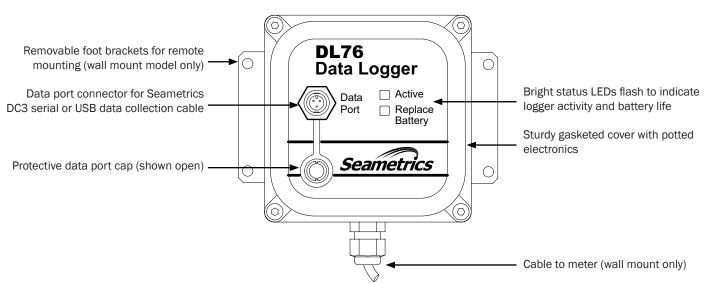

SPECIFICATIONS*

Size C 3.6 Vdc li	Size C 3.6 Vdc lithium battery (included)		
Estimated life is	Estimated life is 3-5 years depending on usage.		
0° to 130° F (-1	0° to 130° F (-18° to 54°C)		
mL, liter, gallon,	mL, liter, gallon, Imperial gallon, cubic foot, cubic meter, million gallon		
Seconds, minute	Seconds, minutes, hours, days		
	Liter, gallon, Imperial gallon, cubic foot, cubic meter, million gallon, acre-foot, acre-inch, megaliter, thousand-gallon		
Capacity	at	Sampling Interval	
11 days	at	15 seconds	
22 days	at	30 seconds	
44 days	at	60 seconds	
6 months	at	240 seconds	
1 year	at	480 seconds	
3 years	at	1450 seconds	
500 Hz			
Low battery; Pow	Low battery; Power		
Selectable optio	Selectable options (Stop or Overwrite)		
10 minutes/mor	10 minutes/month (.02%)		
	Estimated life is 0° to 130° F (-1) multiple mL, liter, gallon, Seconds, minute Liter, gallon, Imp acre-foot, acre-ir Capacity 11 days 22 days 44 days 6 months 1 year 3 years 500 Hz Low battery; Pow	Estimated life is 3-5 years dep 0° to 130° F (-18° to 54° C) mL, liter, gallon, Imperial gallon, or acre-foot, acre-inch, megaliter Capacity at 11 days at 22 days at 44 days at 6 months at 1 year at 3 years at 500 Hz Low battery; Power Selectable options (Stop or Or	

*Specifications subject to change • Please consult our website for current data (www.Seametrics.com).

MOUNTING & CONNECTIONS

MOUNTING


There are three mounting configurations for a DL76: Meter mount for mechanical meters, meter mount for insertion magmeters, and wall mount (DL76W). The meter mount models match up to any Seametrics lower square housing. All configurations can be factory-ordered or field-installed. Converting from one mounting configuration to another requires use of MK10 or MK20 mounting kits.

OPERATION

Seametrics FlowInspector V.2 software is required for operation of the DL76. Please consult your FlowInspector manual for instructions in loading the software onto your **Meter Mounting.** Remove the four screws on the meter cover with a 5/32" Allen wrench. After connecting the leads to their respective terminals (see diagram), put the DL76 in place of the meter cover and tighten the screws evenly. The gasket on the DL76 should be visibly compressed by tightening all around.

computer, setting up your DL76 for use, downloading, storing, and analyzing your data.

DIMENSIONS

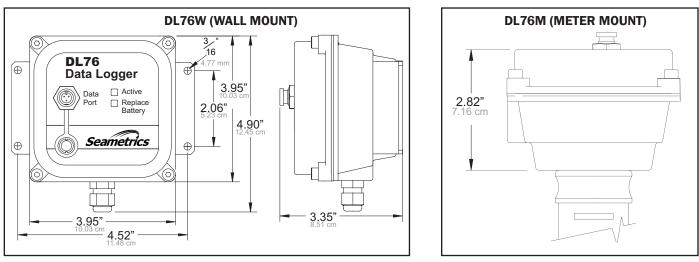


CONNECTIONS (see also next page)




Caution: Do not apply external power to the DL76

DL76 TO MECHANICAL METER

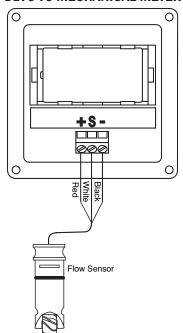


DL76 TO MAGMETER

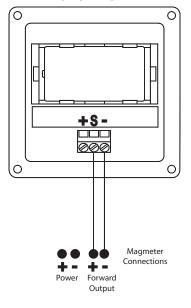


CONNECTIONS

DL76 TO FT415

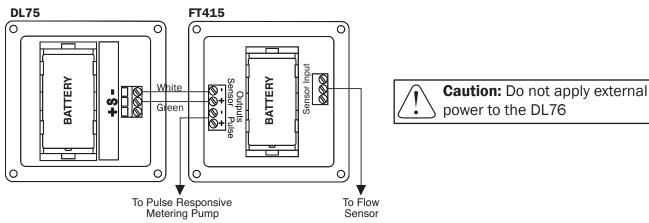

DL76 T0 FT420

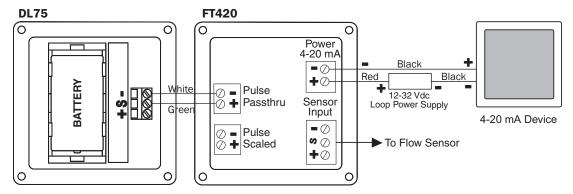

TROUBLESHOOTING

Problem	Probable Cause	Try
Laptop screen reads "No connection" and "Ac- tive" light is NOT blinking	DL76 is transmitting data. Wait two minutes before taking action.	Wait for "Active" light to blink
	Dead battery in DL76	Replace battery
Laptop screen reads "No connection," but "Ac- tive" light <u>IS</u> blinking	Loose cable	Tighten cable
	Bad cable	Test cable (tech bulletin "DL75/76: Testing the DC3 Serial Cable" on Downloads page at www.Seametrics.com)
Flow rate incorrect	K-factor setting is incorrect	Make sure K-factor in DL76 matches flow sen- sor
No flow rate	Damaged flow sensor	Mechanical: See if rotor spins freely EX Magmeter: See if "Status LED" indicator is blinking
	Broken wire	Check for flow rate



Seametrics Incorporated • 19026 72nd Avenue South • Kent, Washington 98032 • USA (P) 253.872.0284 • (F) 253.872.0285 • 1.800.975.8153 • www.Seametrics.com